




Titanium Grade 5

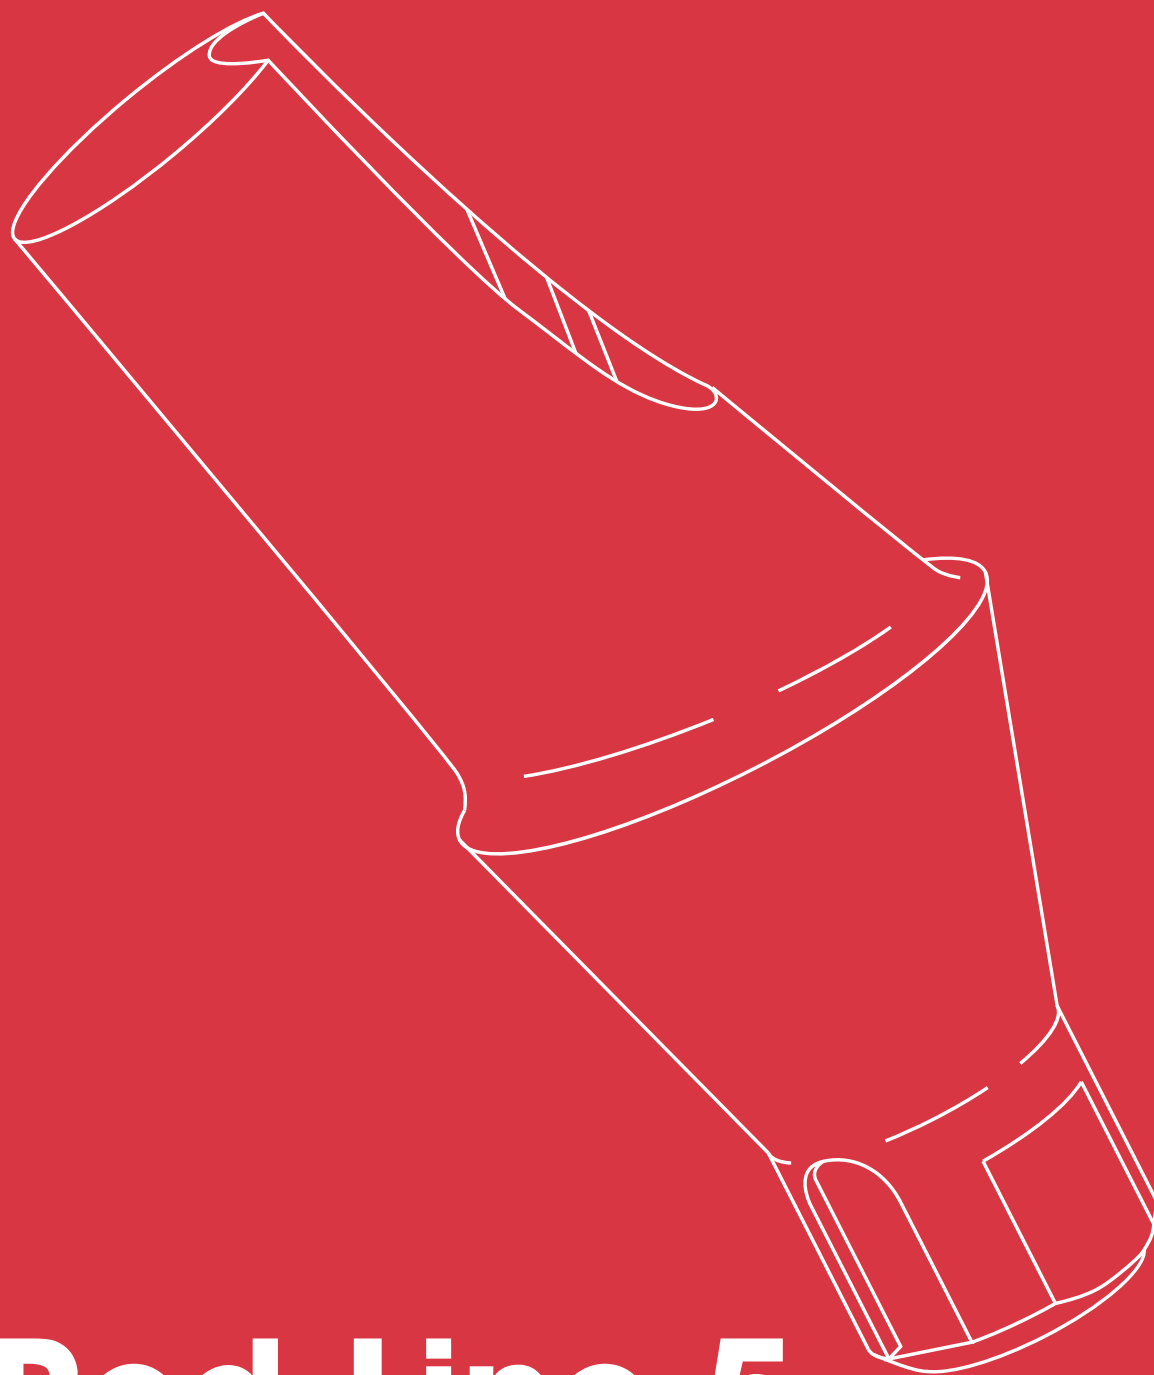

05.100

# Red Line.5

Prosthetic components compatible with  
**STRAUMANN BONE LEVEL® implants**

# Red Line.5

Titanium grade 5

Prosthetic components compatible with  
STRAUMANN BONE LEVEL® implants

## Healing Screws.



Ref. Number      Diameter  $\varnothing$       Height (mm)

05.330.403	Yellow	3.3	3
05.330.405	Yellow	3.3	5
05.410/480.403	Purple	4.1/4.8	3
05.410/480.405	Purple	4.1/4.8	5

## Lab Analogs.



Ref. Number      Diameter  $\varnothing$

05.330.200	Yellow	3.3
05.410/480.200	Purple	4.1/4.8

\* Only one lab analog for both methods  
(impression or scanning)

## Impression Posts.



Ref. Number      Diameter  $\varnothing$       Impression Method

05.330.500	Yellow	3.3	Open Tray
05.330.550	Yellow	3.3	Closed Tray
05.410/480.500	Purple	4.1/4.8	Open Tray
05.410/480.550	Purple	4.1/4.8	Closed Tray

◆ Screw Ref. Number:

Open Tray: 05.330.500.100 / 05.410/480.500.100

Closed Tray 05.100

## Scan Bodies.



Ref. Number      Diameter  $\varnothing$

05.330.SA	Yellow	3.3
05.410/480.SA	Purple	4.1/4.8

◆ Screw Ref. Number: 05.100

\* Novamind scan bodies are used only in combination to novamind free libraries either with novamind ti-bases or directly on implant restorative platforms. Scan Bodies are made of peek and are easily scanned with intra-oral and desktop scanners.

Prosthetic components compatible with  
**STRAUMANN BONE LEVEL®** implants

## Ti-Bases.



Anti-Rotation



No Anti-rotation

Ref. Number      Diameter  $\varnothing$       Gingiva Height (mm)

	05.330.600.10	3,3	1
	05.330.600.20	3,3	2
	05.330.601.10	3,3	1
	05.330.601.20	3,3	2
	05.410/480.600.10	4,1/4,8	1
	05.410/480.600.20	4,1/4,8	2
	05.410/480.601.10	4,1/4,8	1
	05.410/480.601.20	4,1/4,8	2

Screw Ref. Number: 05:100

Novamind TI-BASES are colored with a warm Golden Hue for better aesthetic effect. They are available in two types, with and without antirotation depending on the type of restoration (crown or bridge)

## Titanium Abutments for Cemented Restorations.



Ref. Number      Diameter  $\varnothing$       Angulation Degrees(°)      Gingiva Height (mm)

05.330.00.120	3,3	0°	1,2
05.330.00.270	3,3	0°	2,7
05.330.17.120	3,3	17°	1,2
05.330.17.270	3,3	17°	2,7
05.330.23.120	3,3	23°	1,2
05.330.23.270	3,3	23°	2,7
05.410/480.00.120	4,1/4,8	0°	1,2
05.410/480.00.270	4,1/4,8	0°	2,7
05.410/480.17.120	4,1/4,8	17°	1,2
05.410/480.17.270	4,1/4,8	17°	2,7
05.410/480.23.120	4,1/4,8	23°	1,2
05.410/480.23.270	4,1/4,8	23°	2,7

Screw Ref. Number: 05:100

Available in different degrees of angulation 0°, 17°, 23°. Two different gingiva height collars to optimize the best possible emergence profile.

## Castable Abutments.



Ref. Number      Diameter  $\varnothing$

	05.330.300	3,3
	05.330.301	3,3
	05.330.710	3,3
	05.330.711	3,3
	05.410/480.300	4,1/4,8
	05.410/480.301	4,1/4,8
	05.410/480.710	4,1/4,8
	05.410/480.711	4,1/4,8



Anti-Rotation



No Anti-rotation



Two types of castable abutments are available. One is fully plastic and one is with pre-fabricated Co-Cr implant connection for cast-on.

Screw Ref. Number: 05:100

# Red Line.5

Titanium grade 5

Prosthetic components compatible with  
**STRAUMANN BONE LEVEL®** implants

## Overdenture Over-Lock Abutments.

Ref. Number      Diameter  $\varnothing$       Height (mm)



05.330.801	3.3	1
05.330.802	3.3	2
05.330.803	3.3	3
05.330.804	3.3	4
05.410/480.801	4.1/4.8	1
05.410/480.802	4.1/4.8	2
05.410/480.803	4.1/4.8	3
05.410/480.804	4.1/4.8	4

\* Over-Locks are compatible to locator abutments for overdentures. 4 different Heights.

## Overlock Standard Retention Kit.

Description

Reference Number



Metal Housing	MH800
Black Lab Plastic	PL.800.BLACK
Blue Plastic Light Retention 0.68 KG	PL.800.BLUE
Grey Plastic Medium Retention 1.36 KG	PL.800.GREY
Clear Plastic Strong Retention 2.26 KG	PL.800.CLEAR

\* Available either as a set or individually. They are used in cases where the total angulation axis among implants does not exceed 15°.

## Overlock Extended Retention Kit with no Core.

Description

Reference Number



Metal Housing	MH800
Black Lab Plastic	PL.800.BLACK
Red Plastic Light Retention 0.68 KG	PL.800.RED
Orange Plastic Medium Retention 1.36 KG	PL.800.ORANGE
Green Plastic Strong Retention 2.26 KG	PL.800.GREEN

\* Available either as a set or individually. They are used in cases where the total angulation axis among implants exceeds 15°.

Prosthetic components compatible with  
**STRAUMANN BONE LEVEL®** implants

## Titanium Temporary Cylinders.



Ref. Number	Diameter $\varnothing$
05.330.900	3.3
05.330.901	3.3
05.410/480.900	4.1/4.8
05.410/480.901	4.1/4.8

◆ Screw Ref. Number: 05.100

Anti-Rotation

No Anti-rotation

\* Chairside use or indirect in lab. With and without antirotation depending on the type of restoration (crown or bridge). Golden warm hue for better aesthetics.

## Multi-Unit Abutments.



Ref. Number	Diameter $\varnothing$	Angulation Degrees(°)	Gingiva Height (mm)
MU.05.330.00.100	3.3	0°	1.0
MU.05.330.00.200	3.3	0°	2.0
MU.05.330.00.300	3.3	0°	3.0
MU.05.330.00.400	3.3	0°	4.0
MU.05.330.17.250	3.3	17°	2.5
MU.05.330.17.350	3.3	17°	3.5
MU.05.330.30.350	3.3	30°	3.5
MU.05.330.30.450	3.3	30°	4.5
MU.05.410/480.00.100	4.1/4.8	0°	1.0
MU.05.410/480.00.200	4.1/4.8	0°	2.0
MU.05.410/480.00.300	4.1/4.8	0°	3.0
MU.05.410/480.00.400	4.1/4.8	0°	4.0
MU.05.410/480.17.250	4.1/4.8	17°	2.5
MU.05.410/480.17.350	4.1/4.8	17°	3.5
MU.05.410/480.30.350	4.1/4.8	30°	3.5
MU.05.410/480.30.450	4.1/4.8	30°	4.5

◆ Screw Ref. Number: 05.100

\* Multi-unit abutments is currently the most accepted and highly recommended solution in screw retained restorations. They have many advantages such as a common prosthetic platform for all implants.

# Red Line.5

Titanium grade 5

Prosthetic components compatible with  
**STRAUMANN BONE LEVEL®** implants

## Multi-Unit Prosthetic System.

Description

Reference Number



Healing Screw	MU.402
Impression Post Open Tray	MU.500
Scan Abutment	MU.SA
Lab Analog	MU.200
Plastic Castable	MU.301
Ti-Base	MU.601
Titanium Temporary Cylinder	MU.901

◆ **Screw Ref. Number:** MU.500.100  
MU.100

\* **Multi-Unit has its own prosthetic components, the same for all implant systems.**